
Status of radiographic services at government hospitals in Gaza Governorates, Palestine

Yasser Alajerami*, Suleiman Maher,
Abushab Khaled and Najim Ahmed

Department of Medical Imaging,
Al-Azhar University,
Gaza Strip, Palestine
Email: yasser_ajr@hotmail.com
Email: mdas111@hotmail.com
Email: khaledshap@hotmail.com
Email: ahmednajim99@yahoo.com
*Corresponding author

Abstract: The complex situation of the current health services exists to shift the system in significant ways to improve on this situation. The radiographic services need more efforts for building capacity. This study is conducted to evaluate radiographic services at government hospitals in Gaza Governorates. Triangulated study design was used for data collection. In the quantitative part, 170 radiological technologists completed questionnaires with 95.5% response rate. The researcher used arbitrated checklist to evaluate medical imaging facilities. Census study was conducted on all radiological technologists and medical imaging departments at six main government hospitals in the Gaza Strip. In addition, three key informant interviews with radiological technologist managers were conducted. Researchers directly interviewed 170 participants. Findings revealed that there was shortage in number of radiographic equipment and radiological technologists. Generally, radiographic departments that followed standard in structure were 45%. Regarding fluoroscopic rooms, 79% of structure followed the standard. The majority of existing darkrooms fulfilled the international standard. An improvement in human resources among medical imaging facilities was clearly observed after 1996. An observable shortage is seen in number of radiographic machines and radiological technologists at all government hospitals. All departments revealed clear defects in structure, design and essential supplies.

Keywords: radiographer; Gaza; triangulated study; darkrooms.

Reference to this paper should be made as follows: Alajerami, Y., Maher, S., Khaled, A. and Ahmed, N. (2018) 'Status of radiographic services at government hospitals in Gaza Governorates, Palestine', *Int. J. Low Radiation*, Vol. 11, No. 1, pp.78–88.

Biographical notes: Yasser Alajerami is Associate Professor in Medical Imaging Department, especially in radiation protection and radiotherapy techniques. He gained his PhD degree in Radiation Protection from University of Technology Malaysia (UTM).

Suleiman Maher is Head of CT Department, Indonesia Hospital. She graduated the public health from Al Quds University. Her work is focused on studying the effect of low ionising radiation on biological tissues.

Abushab Khaled is Associate Professor in Medical Imaging Department, especially in Nuclear Medicine and radiation protection. He gained his PhD degree in Nuclear Medicine from Universidad Complutense de Madrid, Madrid, Spain.

Najim Ahmed is Associate Professor in Nursing Department, especially in Public Health and Advanced Nursing Techniques. He gained his PhD from Cairo University, Egypt.

This paper is a revised and expanded version of a paper entitled 'Evaluation of medical imaging services at government hospital in Gaza Governorates' presented at the 'International Conference of Applied Medical Sciences (ICAMS-2017)', Gaza City, Palestine, 18–19 November 2017.

1 Introduction

Healthcare system in Palestine is complex, because health service delivery in Palestine is divided into five major healthcare providers: two public providers (the Ministry of Health and the Ministry of Interior – military health services), multiple private providers (hospitals, clinics) and numerous NGO providers (the United Nations Relief and Works Agency and other local NGOs). The main provider MOH is operating 25 hospitals and 448 PHC facilities, 394 in West Bank (WB) and 54 in Gaza Strip (GS) (PCBS, 2015; MOH, 2015; Abushab et al., 2017).

MOH is the main provider of secondary care in the GS. It is responsible for 13 hospitals across the five governorates and the number of hospital beds in the GS is about 2037 and percentage of hospital beds per 1000 capita is about 1.2 (MOH, 2015). The average occupancy rate at hospitals in the GS is about 88%. The unstable Palestinian political situation increases the load on the healthcare services in Gaza and West Bank.

Substantial effect in diagnosis and treatment of different diseases is attributed to the medical imaging services. The medical imaging services are a critical part of healthcare provision for patients at all of the three levels of healthcare (primary, secondary, and tertiary) especially in secondary care. The MOH is the main provider of the medical imaging services in Palestine, where the number of radiological examinations in the GS reached 519,220. The majority of these exams (81%) were conducted at governmental hospitals in the GS. These services are represented as the following: conventional radiography 78.6%, Computed Tomography (CT) 6.2%, Magnetic Resonance Imaging (MRI) 0.7%, fluoroscopy 0.8%, and others 13.7%. A significant increase is seen in medical imaging services in the GS between 2006 and 2014 (MOH, 2015).

No previous study about evaluation of medical imaging services in the GS was reported. Evaluation of medical imaging services is very important particularly in the GS, which is politically instable, suffering poverty and low health resources. This study conducted to evaluate basic radiographic services (conventional X-ray, fluoroscopy and processing room) at government hospitals in the GS.

2 Methods

2.1 Study design

The design of this study was descriptive, analytical cross-sectional one with a triangulated design (quantitative and qualitative).

2.2 Study population and data collection

The current study was conducted on six main targets; medical imaging equipment, human resources and department designs. All designs, RTs and equipment of radiographic departments at the six main governmental hospitals were evaluated based on international standards and reports.

The quantitative part was collected from the radiographic departments. With regard to the qualitative part, in-depth interviews were accompanied with three key informant managers from the medical imaging administration of governmental hospital.

The first part presented characteristic data about the participants, which was personal and work related data: age, gender, residency place, qualification, training courses, years of experience, hospital name...etc. The second part demonstrated equipment information about basic radiographic services. The data included: machine numbers, machine types, machine status, maintenance checkup, annual breakdown and image types. The second type of data collection was checklist develop by the researcher based on international standards 'Australasian Health Facility Guidelines (2016)', 'radiological protection Institute of Ireland' and 'National Health Services'.

The key informant interviews were used as a third data collection method. Semi structured, open-ended statements were performed. Three experts were selected to conduct in-depth interviews to dig beneath the elicited quantitative data, make deep understanding and generate new ideas, and give more evidence towards their perception.

2.3 Ethical consideration

The study approval was received from Al-Azhar University, and an official letter of approval from the Helsinki committee in Gaza was obtained.

3 Results

3.1 General information about existing radiographic department

Table 1 shows readings for Gaza: governorates number, hospitals establishment, hospital area, employees, RTs and beds number in the six main governmental hospitals (Al-Shifa, European Gaza, Indonesia, Shohda Al-Aqsa, Nasser, and Abu Yousef Al Najjar Hospital).

Table 1 Distribution of main six government hospitals in the GS

<i>Hospital name</i>	<i>Item</i>	<i>Governorate</i>	<i>Establishment</i>	<i>Area (m²)</i>	<i>Employees number</i>	<i>Radiologists number</i>	<i>RTs number</i>	<i>Beds number</i>
Indonesia		North	2015	16,000	350	4	20	110
Al-Shifa		Gaza	1946	45,000	1535	20	55	583
Shohda Al-Aqsa		Mid Zone	2001	4000	474	3	21	261
European Gaza		Khan Younis	2000	56,000	691	11	29	261
Nasser		Khan Younis	1960	25,000	880	6	28	330
Abu Yousef Al Najjar		Rafah	2000	4000	297	3	17	49

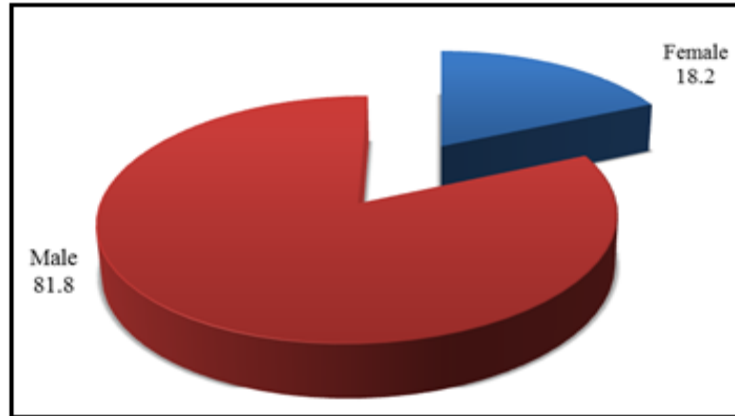
The total number of distributed questionnaires was 176 and the number of respondents was 170 with a response rate of 95.5%. The first section is planned to analyse the demographic characteristics of the study sample (radiological technologists) $N = 170$ including (Name of hospital, Age, Gender, Certificate, Employment, Years of experience, Training).

Table 2 clarifies that 20% of RTs were aged less than 30 years, 55.2% between 30 and 40 years, around 12.4% between 40 and 50 years and the same percentage for those older than 50 years. In addition, around 36.5% of RTs have less than 10 years' experience and 43.5% of them have 10–17 years' experience, while 9.4% of RTs have 17–24 years' experience and 10.6% more than 24 years' experience.

Table 2 Distribution of RTs by characteristics variables ($N = 170$)

<i>Variables</i>		<i>Frequency</i>	<i>%</i>
Gender	Male	139	81.8
	Female	31	18.2
Age groups	< 30 years	34	20.0
	30–40	94	55.2
	40–50	21	12.4
	>50 years	21	12.4
Experience	<10 years	62	36.5
	10–17	74	43.5
	17–24	16	9.4
	>24 years	18	10.6

Regarding to participants' gender, the majority of RTs were males (81.8%), while 18.2% were females as shown in Figure 1.

Figure 1 Distribution of RTs based on gender

3.2 Evaluation designs of existing radiographic department

3.2.1 Conventional radiography design checklist

Table 3 clarifies that all of conventional radiography rooms in medical imaging department have a control console, but only 56.3% of these rooms have proper size ($\geq 1.5 \times 2$ m²) and provided with drainage sewage (Bushong, 2013). Generally, the operator console area allows observing and communicates with the patient during imaging process. This area should be sufficiently large to reduce radiation intensity at the operator's screen and boundaries (MIA, 2017). Around 18.8% of rooms have windows, and toilet inside imaging room.

Table 3 Checklist about structure of conventional radiography in government hospitals

Item	Hospital name		Al-Shifa		European Gaza		Nasser		Shohda Al-Aqsa		Indonesia		Abu Yousef Al Najjar		Total	
	Y	N	Y	N	Y	N	Y	N	Y	N	Y	N	Y	N	Y%	N%
Is control console area suitable? ($\geq 1.5 \times 2$ m)	5	1	2		1	2	1	1			1		2		56.3	43.8
Are there windows for room?	3	3		2		3		2			1		2		18.8	81.2
Is there a toilet inside the room?	3	3		2		3		2			1		2		18.8	81.2
Is a room size at least 30 m ² ?	3	3	2		2	1	1	1			1		2		50	50
Is there drainage sewage?	6			2	1	2	1	1	1				2		56.3	43.8
Is there a changing cubicle?	3	3	2			3		2			1		2		31.3	68.8
The customers/patients door entrance at least 180x150 cm ² ?	3	3		2		3	2				1		2		31.3	68.8

Note: Y = yes; N = no.

The current check showed that 50% of imaging rooms have proper size ($\geq 30 \text{ m}^2$) (MOH, 2015; Bushong, 2013; MIA, 2017). Other international standard exhibited that X-ray room size should be 33 m^2 to contain patient table and the vertical chest bucky stand. The boundaries to all occupied areas (walls, doors, doorframes, floor, ceiling, window and the protective viewing screen) must shield appropriately (NHS, 2001). Finally, 31.3% of the current rooms have a change cubicle and patients' door entrance dimension fit with the international standard ($\geq 180 \times 150 \text{ cm}$). The door should be wide enough and must be shielded against scatter radiation (NHS, 2002; Bushong, 2013).

The location, design and equipment layout of X-ray rooms must carefully consider the radiation protection perspective. This is easier when X-ray facilities are not designed as stand-alone rooms but planned as part of an integrated radiology/imaging department with its supporting areas and services. Planning the room layouts should start as early as possible in the design process. The design of ancillary facilities such as changing cubicles, and toilets should be considered (MIA, 2017).

3.2.2 Fluoroscopy design checklist

Table 4 clarifies that all of fluoroscopic rooms followed the international standard in terms of control consoles and toilets (Bushong, 2013). In addition, 71.4% of these rooms obey the standards in terms of room size ($\geq 36 \text{ m}^2$), have changing cubicle and proper drainage of sewage. Fluoroscopy systems may have large machines operated by remote control, control console and much equipment (Owen et al., 1995; NHS, 2001). Finally, 57.1% of these rooms have a proper patients' door entrance ($\geq 180 \times 150 \text{ cm}$) (Bushong, 2013).

Table 4 Checklist about structure of fluoroscopy at government hospitals

Item	Hospital name		Al-Shifa		European Gaza		Nasser		Shohda Al-Aqsa		Indonesia		Abu Yusef Al Najjar		Total	
	Y	N	Y	N	Y	N	Y	N	Y	N	Y	N	Y	N	Y%	N%
Is there a control console?	2		1		1		1		1		1		1		100	0
Is there a toilet inside the room?	2		1		1		1		1		1		1		100	0
Is a room size at least 36 m^2 ?	2		1		1				1	1			1		71.4	28.6
Is there a changing cubicle?	2		1		1				1	1			1		71.4	28.6
Is there a drainage sewage	2				1	1			1		1		1		71.4	28.6
Are the patient's door entrance at least $180 \times 150 \text{ cm}$? (STD)	2				1		1		1		1		1		57.1	42.9

Note: Y = yes; N = no.

3.2.3 Darkroom design checklist

All darkrooms in medical imaging departments at government hospitals were provided with automatic processing machines except Indonesia Hospital and have computerised system (digitalise images). In the current study, 12 processing machines were available in

government hospitals. These machines were distributed as 4, 2, 2, 2 and 2 in Al-Shifa, Shohda Al-Aqsa, European Gaza, Nasser and Abu Yousef Al Najjar Hospital, respectively. In terms of product type, four machines were 'AGFA product' at Al-Shifa Hospital and eight were 'compact product'. Finally, four computed radiography machines were available at Al-Shifa, European Gaza, Nasser, and Indonesia Hospital.

Table 5 clarifies that all dark rooms in medical imaging departments at governmental hospitals adjacent to imaging rooms. In terms of a room size, half of dark rooms followed the international standard ($\geq 6 \text{ m}^2$) (Bushong, 2013). Around 91.7% of these rooms have drainage sewage, and 83.3% have enough space for developing tanks.

Table 5 Checklist about structure of darkrooms at governmental hospitals

Item	Hospital name		Al-Shifa		European Gaza		Nasser		Shohda Al-Aqsa		Indonesia		Abu Yousef Al Najjar		Total	
	Y	N	Y	N	Y	N	Y	N	Y	N	Y	N	Y	N	Y%	N%
Is the dark room adjacent to imaging rooms?	4		1		2		2		1		2		100	0.0		
Is the room size $\geq 6 \text{ m}^2$?	1	3	1		1	1	1	1	1		1	1	50	50		
Is there drainage sewage?	3	1	1		2		2		1		2		91.7	8.3		
Is there a space for developing tanks?	3	1	1		2		2				1	2	83.3	16.7		

3.3 Evaluation of medical imaging equipment

Table 6 clarifies the availability of the main four imaging equipment (i.e., conventional radiography and fluoroscopy) at governmental hospitals. Starting with Al-Shifa Hospital, five conventional radiography machines are available (the sixth one is used as spare machine) and two fluoroscopic machines (one is used as spare machine).

Table 6 Availability of radiographic machines

Medical imaging machine		Al-Shifa Hospital	European Gaza Hospital	Nasser Hospital	Shohda Al-Aqsa Hospital	Indonesia Hospital	Abu Yousef Al Najjar Hospital	Total
Conventional Radiography	Functioning	5	2	2	2	1	2	14
	Not Functioning	1	0	1	0	0	0	2
Fluoroscopy	Functioning	1	0	1	0	0	1	3
	Not Functioning	1	1	0	1	1	0	4

In Nasser Hospital, there are three conventional radiography machines (two machines work and one is not working) and one fluoroscopic machine. In Shohda Al-Aqsa Hospital, two conventional radiography machines were available and one fluoroscopic machine. Regarding Indonesia Hospital, only one conventional radiography machine and one fluoroscopic machine (not working). Finally, in Abu Yousef Al Najjar Hospital there are two conventional radiography machines, and one fluoroscopic machine.

Table 7 demonstrates the status of X-ray machines compared with the international standard, based on equation (1) (MOH, 2015). The number of X-ray machines is directly proportional to the number of hospital beds.

$$\text{Required no. of X-ray machines} = \frac{\text{No. of hospital beds}}{50} \quad (1)$$

Based on equation (1), it is clear that all hospitals suffer from shortage of X-ray machines. Accordingly, the required number of X-ray machines should be at least 2, 11, 5, 5, 6 and 1 in Indonesia, Al-Shifa, Shohda Al-Aqsa, European Gaza, Nasser and Abu Yousef Al Najjar Hospital, respectively. Currently, the existing X-ray machines in medical imaging departments were 1, 6, 2, 2, 3 and 2, respectively.

Table 7 X-ray machines existing at government hospitals compared to the international standard

<i>Hospital</i>	<i>No. of beds</i>	<i>Required no. of X-ray machines</i>	<i>Existing X-ray machines</i>
Indonesia	110	2.2	1
Al-Shifa	583	11.6	6
Shohda Al-Aqsa	261	5.2	2
European Gaza	261	5.2	2
Nasser	330	6.6	3
Abu Yousef Al Najjar	49	1	2

3.4 Evaluation of RTs in governmental hospitals

Table 8 demonstrates number of RTs in conventional radiographic rooms at government hospitals and number of daily exams. At the morning shift, number of RTs worked at morning shift was 5, 7, 8, 7, 7, 12 in European Gaza, Indonesia, Shohda Al-Aqsa, Nasser and Al-Shifa Hospital, respectively. Based on these values, each RT at the morning shift will carry out 24, 21, 18, 23, 18 and 23 exams, respectively. In parallel, number of RTs worked at evening shift was 5, 2, 4, 3, 2, 4 in European Gaza, Indonesia, Shohda Al-Aqsa, Nasser and Al-Shifa Hospital, respectively. Thus, each RT at the evening shift will carry out 16, 50, 18, 30, 45 and 63 exams, respectively.

In Al-Shifa Hospital, each RT conducted 23 and 63 exams at morning and evening shift. This imaging value considers the largest percentage compared to the other hospitals especially at the evening shift. For example, RT at Al-Shifa Hospital suspected to radiograph four times more than the RT in European Gaza Hospital.

Table 8 Number of daily examinations to the number of RTs in conventional radiography

<i>Item</i>	<i>Hospital</i>					
	<i>EGH</i>	<i>Indonesia</i>	<i>S. Al-Aqsa</i>	<i>Nasser</i>	<i>A. Al Najjar</i>	<i>Al-Shifa</i>
Number of RTs at morning shift	5	7	8	7	7	12
Number of exams at morning shift	120	150	145	160	125	270
The number of examination for each RT in morning shift	24	21	18	23	18	23
Number of RTs at evening & night shift	5	2	4	3	2	4
Number of exams at evening & night shift	80	100	70	90	90	250
The number of examination for each RT in evening shift	16	50	18	30	45	63

Table 9 demonstrates the ratio of RTs to the number of daily fluoroscopic exams at government hospitals. At the morning shift, each fluoroscopic room, in all hospitals, has only one RT. Based on these readings, each RT at the morning shift will carry out 7, 1, 9 exams in Nasser, Abu Yousef Al Najjar and Al-Shifa Hospital, respectively. Regarding the evening shift, only Al-Shifa Hospital provides fluoroscopic exams with one suspected case daily.

Table 9 Number of daily examinations to the number of RTs in fluoroscopy

<i>Item</i>	<i>Hospital</i>		
	<i>Nasser</i>	<i>Abu Yousef AL Najjar</i>	<i>Al-Shifa</i>
Number of RTs at morning shift	1	1	1
Number of exams at morning shift	7	1	9
The number of examination for each RT in morning shift	7	1	9
Number of RTs at evening & night shift	0	0	1
Number of exams at evening & night shift	0	0	1
The number of examination for each RT in evening shift	0	0	1

3.5 *The relationship between patient waiting time and number of exams at morning shifts in conventional radiography*

Table 10 illustrates correlation between patient waiting time and number of exams at morning shift in conventional radiography by using Pearson correlation test. The value of correlation coefficient was 0.779 and p -value was 0.000 (>0.05). This result indicates that there is statistically significant relationship between the tested variables at significance level $\alpha \leq 0.05$. When number of exams increases, patient-waiting time will consequently increase. Actually, the patient-waiting time can reduced by increasing the number of radiographic machines.

Table 10 The relationship between patient waiting time and number of exams at morning shifts in conventional radiography

<i>Items</i>	<i>Test Statistic</i>	<i>P-value</i>
The relationship between patient waiting time and number of exams at morning shift	0.779	0.000*

Note: *Correlation is significant at the 0.05 level (2-tailed).

4 Discussion

The current results showed that around 75% of the RTs are aged less than 40 years and around 25% older than 40 years. It is known that medical imaging services need special effort, skill and tolerance (heavy-duty and experience). The current readings presented multiplicity in ages of RTs, which facilitate process of department's management. In addition, around 86.5% of RTs were permanent employees, 10.0% of them were contracts, and six (3.5%) were volunteers.

Regarding RTs, gender, the current results are completely different from the international readings (60–70% female and 30–40% male) (PCBS, 2015).

Regarding rooms that have windows, they are only at Al-Shifa Hospital at different height levels without lead shielding. According to the international standard, no window should be in radiographic room and if these windows exist they must be lead shielded.

Regarding changing cubicles, they should be close to X-ray room and may be designed as individual changing rooms, which open directly into the X-ray room. This will allow for changing arrangements consistent with good radiation protection practice, greater privacy, security and perhaps faster patient throughput (MIA, 2017).

No medical imaging department fulfils the international standard. In the GS, several difficulties and obstacles are faced in the developing of medical facilities, particularly the medical imaging field. These obstacles are related to high cost of equipment and siege imposed on the GS. Finally, the occupation prohibited the import of equipment and related spare boards and parts (RPII, 2009).

Regarding fluoroscopic rooms, it is well known that the radiation dose of fluoroscopic machines is significant and higher than X-ray machines. A serious problem was observed at Al-Shifa Hospital. Thus, RT at this hospital suspected to perform 2 to 8 cases more than Nasser and Abu Yousef Al Najjar Hospital, respectively. Consequently, duplication in radiation dose is highly expected for RTs at Al-Shifa Hospital compared to other hospitals.

5 Conclusion

Radiographic departments in the government hospitals were evaluated based on international standards. The evaluation was conducted based on several questions through face-to-face interview with the RTs at government hospitals, and through personal interview with medical imaging administration. The number of RTs was dramatically increased (~5 times more) during the last twenty years. Four-fifths of RTs were males and aged less than 40 years. Significant overload on RTs was remarked in all medical imaging departments at governmental hospitals, especially at evening and night

shift. Statistically significant relations were observed between excess number of exams at morning shift and patient waiting time in conventional radiography.

Regarding conventional X-ray machines, 16 machines were available and almost all ready for use; five fluoroscopic machines were obtainable, but about half were not functioning. Comparing with the international standards, there was shortage in number of X-ray machines at all medical imaging departments.

In conclusion, around 45% of all conventional radiography structure at government hospitals adopted the international standard and 74% of radiographic equipments are functioning. Regarding fluoroscopy rooms and darkrooms, 79% and 81% followed the standard, respectively.

Acknowledgement

This paper received special funding from IBHATH project from Qatar Charity Institute.

References

- Abushab, K.M., Suleiman, M.D., Alajeramim, Y.S.M., Alagham, S.I., Alnahalm, M., Najimm, A. and Naserm, M. (2017) 'Evaluation of advanced medical imaging services at Governmental Hospitals-Gaza Governorates, Palestine', *Journal of Radiation Research and Applied Sciences*, Vol. 11, No. 1, pp.43–48.
- Australasian Health Facility Guidelines (AusHFG) (2016) 'University of New South Wales (UNSW) and Health Capital and Asset Management Consortium (HCAMC)', *Centre for Health Assets Australasia (CHAA) Faculty of the Built Environment UNSW*, Sydney, Australia.
- Bushong, S. (2013) *Radiologic Science for Technologists*, Elsevier Mosby, USA.
- Medical Imaging Administration (MIA) (2017) *Interview with Chief of Radiologic Technologists at governmental hospitals (Ibrahim Abas) and Radiologic Technologist advisors (Rafat Ahmed and Zeiyad Alawour) in the Gaza Strip*, Interview by researcher at January 2017.
- Ministry of Health (MOH) (2015) *Annual report of mortality in the Gaza Strip*, Palestine Health Information System, Gaza, Palestine.
- National Health Service (NHS) (2001) *Facilities for Diagnostic Imaging and Interventional Radiology*, National Health Service, HBN 6, NHS Estates, London Stationery Office.
- National Health Service (NHS) (2002) *Diagnostic Imaging: PACS and Specialist Imaging*, HBN 6 Volume 2, NHS Estates, London Stationery Office.
- Owen, J., Chan, W., Sunshine, J. and Shatter, K. (1995) 'The sex ratio of American radiologists: comparison and implications by age, subspecialty, and type of practice', *American Journal of Roentgenology*, Vol. 165, No. 6, pp.1337–1341.
- Palestinian Central Bureau of Statistics (PCBS) (2015) *Population, Housing units, Building and Establishment*, Palestinian Central Bureau of Statistics, Ramallah, Palestine.
- Radiological Protection Institute of Ireland (RPII) (2009) *The design of diagnostic medical facilities where ionising radiation is used*, RPII in liaison with the principle contributors from St. James's Hospital, Dublin.